

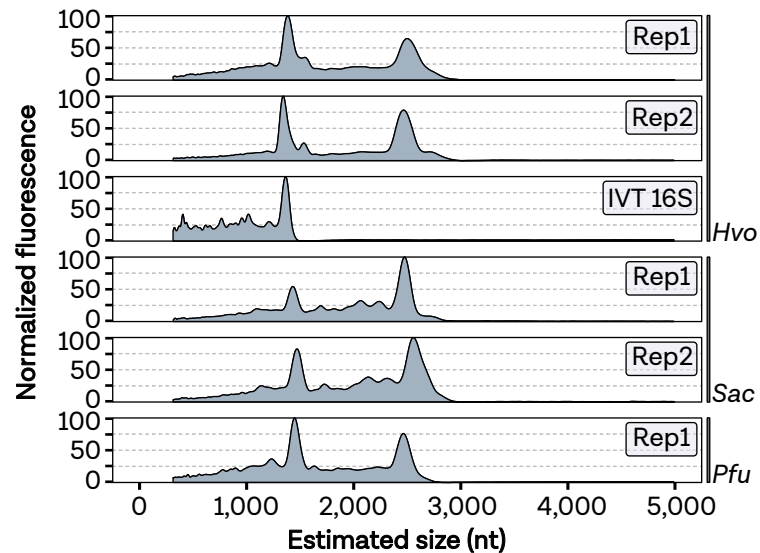
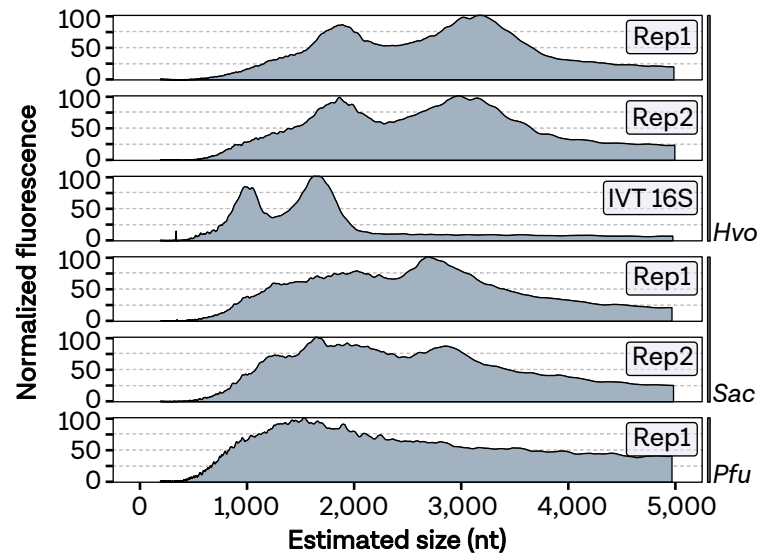
A**B**

Fig. S1 | Bioanalyzer profiles.

A, Bioanalyzer profile of pre-treated RNA used as input for the direct cDNA protocol and **B**, quality control of the cDNA during library preparation.